

## Mouse Total Complement C3 ELISA Kit

Catalog No. **CS531A**  
**CS531B**

Quantity: **1 x 96 tests**  
**5 x 96 tests**

<b>Sensitivity:</b>	0.168 ng/ml MDD
<b>Specificity:</b>	Mouse Complement C3 total antigen
<b>Range:</b>	0.20 - 100 ng/ml
<b>Sample Type:</b>	Serum, plasma, cell supernatants.
<b>Cross-Reactivity:</b>	Does not significantly cross react with human, Porcine, rabbit, sheep, canine, or horse.

**Background:** Complement Component 3 (C3), the most abundant serum complement component, is a disulfide-linked 185 kDa 1,637 amino acid glycoprotein which supports the classical, alternative, and lectin pathways of complement activation. C3 is proteolytically activated by C3-convertase to the anaphylatoxin C3a and the opsonizing agent C3b. Serum concentrations of C3 are increased during acute and chronic inflammation such as rheumatoid arthritis, and are decreased due to increased consumption or autoimmune disorders such as systemic lupus erythematosus.

**Assay Principle:** Mouse C3 will bind to the capture antibody coated on the microtiter plate. After appropriate washing steps, peroxidase labeled polyclonal anti-mouse C3 antibody binds to the captured protein. Excess antibody is washed away and TMB substrate is used for color development at 450 nm. A standard calibration curve is prepared along with the samples to be measured using dilutions of mouse C3. Color development is proportional to the concentration of C3 in the samples.

**Reagents Provided:**

- 96-well antibody coated microtiter strip plate** (wells 8 x 12) containing anti-mouse C3 antibody, blocked and dried.
- 10X Wash Buffer:** 1 bottle of 50 ml
- Mouse C3 standard:** 1 vial lyophilized standard
- Horseradish peroxidase-conjugated anti-mouse C3 primary antibody:** 1 vial lyophilized polyclonal antibody
- TMB substrate solution:** 1 bottle of 10 ml solution

**Storage and Stability:** Store all kit components at 4°C upon arrival. Return any unused microplate strips to the plate pouch with desiccant. Reconstituted standards and primary may be stored at -80°C for later use. Do not freeze-thaw the standard and primary antibody more than once. Store all other unused kit components at 4°C. This kit should not be used beyond the expiration date.

**Reagents and Equipment Required:**

- Microtiter plate shaker capable of 300 rpm uniform horizontally circular movement
- Manifold dispenser/aspirator or automated microplate washer
- Microplate reader capable of measuring absorbance at 450 nm
- Pipettes and Pipette tips
- Deionized or distilled water
- Polypropylene tubes for dilution of standard
- Paper towels or laboratory wipes
- 1N H<sub>2</sub>SO<sub>4</sub> or 1 N HCl



**Cell Sciences®**  
65 Parker Street  
Unit 11  
Newburyport, MA 01950

Toll Free: 888 769-1246  
Phone: 978 572-1070  
Fax: 978 992-0298

E-mail: [info@cellsciences.com](mailto:info@cellsciences.com)  
Web Site: [www.cellsciences.com](http://www.cellsciences.com)

## Mouse Total Complement C3 ELISA Kit

- Bovine Serum Albumin Fraction V (BSA)
- Tris(hydroxymethyl) aminomethane (Tris)
- Sodium Chloride (NaCl)

### Precautions:

- Do not mix any reagents or components of this kit with any reagents or components of any other kit. This kit is designed to work properly as provided.
- Always pour peroxidase substrate out of the bottle into a clean test tube. Do not pipette out of the bottle as contamination could result.
- Keep plate covered except when adding reagents, washing, or reading.
- DO NOT pipette reagents by mouth and avoid contact of reagents and specimens with skin.
- DO NOT smoke, drink, or eat in areas where specimens or reagents are being handled

### Preparation of Reagents:

- TBS buffer: 0.1 M Tris, 0.15 M NaCl, pH 7.4
- Blocking buffer (BB): 3% BSA (w/v) in TBS
- 1X Wash buffer: Dilute 50 ml of 10X wash buffer concentrate with 450ml of deionized water

### Sample Collection:

Collect plasma using EDTA or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000xg within 30 minutes of collection. Assay immediately or aliquot and store at  $\leq -20^{\circ}\text{C}$ . **Avoid repeated freeze-thaw cycles.**

### Assay Procedure:

Perform assay at room temperature. Vigorously shake plate (300rpm) at each step of the assay

Preparation of Standard: Reconstitute standard by adding 1ml of blocking buffer directly to the vial and agitate gently to completely dissolve contents. This will result in a 1,000 ng/ml stock solution.

### Dilution table for preparation of mouse C3 standard curve.

*Once all standard curve dilutions are made, apply immediately to the plate with samples.*

C3 concentration (ng/ml)	Dilution
100	900 $\mu\text{l}$ (BB) + 100 $\mu\text{l}$ (from vial)
50	500 $\mu\text{l}$ (BB) + 500 $\mu\text{l}$ (100ng/ml)
20	600 $\mu\text{l}$ (BB) + 400 $\mu\text{l}$ (50ng/ml)
10	500 $\mu\text{l}$ (BB) + 500 $\mu\text{l}$ (20ng/ml)
5	500 $\mu\text{l}$ (BB) + 500 $\mu\text{l}$ (10ng/ml)
2	600 $\mu\text{l}$ (BB) + 400 $\mu\text{l}$ (5ng/ml)
1	500 $\mu\text{l}$ (BB) + 500 $\mu\text{l}$ (2ng/ml)
0.5	500 $\mu\text{l}$ (BB) + 500 $\mu\text{l}$ (1ng/ml)
0.2	600 $\mu\text{l}$ (BB) + 400 $\mu\text{l}$ (0.5ng/ml)
0	500 $\mu\text{l}$ (BB) Zero point to determine background



## Mouse Total Complement C3 ELISA Kit

### Standard and Unknown Addition:

Remove microtiter plate from bag and add 100  $\mu$ l C3 standards (in duplicate) and unknowns to wells. Carefully record position of standards and unknowns. Shake plate at 300rpm for 30 minutes. Wash wells three times with 300  $\mu$ l wash buffer. Remove excess wash by gently tapping plate on paper towel or kimwipe.

NOTE: The assay measures total mouse C3 in the 0.2-100 ng/ml range. Samples giving mouse C3 levels above 200 ng/ml should be diluted in blocking buffer before use. A 1:100,000 to 1:800,000 dilution for normal plasma and serum samples is suggested for best results.

### Primary Antibody Addition:

Reconstitute primary antibody by adding 10 ml of blocking buffer directly to the vial and agitate gently to completely dissolve contents. Add 100  $\mu$ l to all wells. Shake plate at 300 rpm for 30 minutes. Wash wells three times with 300  $\mu$ l wash buffer. Remove excess wash by gently tapping plate on paper towel or kimwipe.

### Substrate Incubation:



Add 100  $\mu$ l TMB substrate to all wells and shake plate for 5-10 minutes. Substrate will change from colorless to different strengths of blue. Quench reaction by adding 50 $\mu$ l of 1N H<sub>2</sub>SO<sub>4</sub> or HCl stop solution to all wells when samples are visually in the same range as the standards. Add stop solution to wells in the same order as substrate upon which color will change from blue to yellow. Mix thoroughly by gently shaking the plate.

### Measurement:

Set the absorbance at 450 nm in a microtiter plate spectrophotometer. Measure the absorbance in all wells at 450 nm. Subtract zero point from all standards and unknowns to determine corrected absorbance ( $A_{450}$ ).

### Calculation of Results:

Plot  $A_{450}$  against the amount of C3 in the standards. Fit a straight line through the linear points of the standard curve using a linear fit procedure if unknowns appear on the linear portion of the standard curve. Alternatively, create a standard curve by analyzing the data using a software program capable of generating a four-parameter logistic (4PL) curve fit. The amount of C3 in the unknowns can be determined from this curve. If samples have been diluted, the calculated concentration must be multiplied by the dilution factor. Typical standard curves for EXAMPLE ONLY:

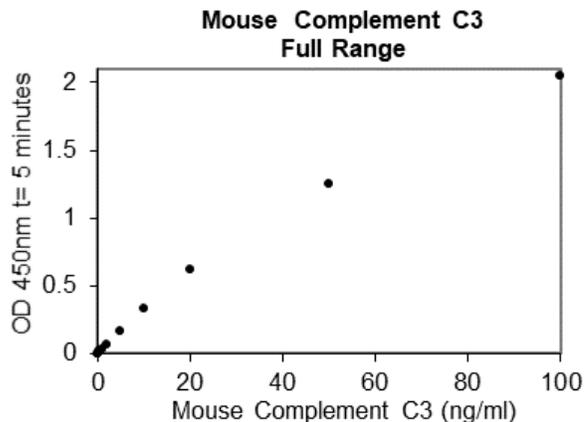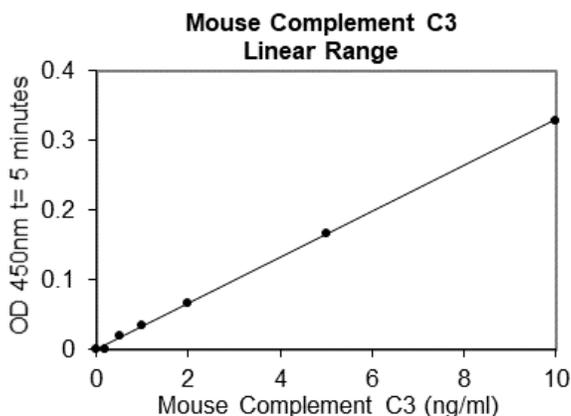

## Mouse Total Complement C3 ELISA Kit

**Expected Values:** C3 in normal mouse plasma ranges from 0.18-1.26 mg/ml (n=8) with an average concentration of 0.54 mg/ml or 1.0 mg/ml.

### Performance Characteristics:

**Sensitivity:** The minimum detectable dose (MDD) was determined by adding two standard deviations to the mean optical density value of the zero standard replicates (range OD<sub>450</sub>: 0.045-0.052) and calculating the corresponding concentration. The MDD was 0.119 ng/ml

**Intra-assay Precision:** Three samples of known concentration were tested 20 times on one plate to assess intra-assay precision.

Sample	1	2	3
n	20	20	20
Mean (ng/ml)	1.56	5.20	27.1
Standard Deviation	0.076	0.102	1.06
CV (%)	4.87	1.96	3.92

**Inter-assay Precision:** Three samples of known concentration were tested in 10 independent assays to assess inter-assay precision.

Sample	1	2	3
n	10	10	10
Mean (ng/ml)	1.62	5.67	27.2
Standard Deviation	0.091	0.276	1.39
CV (%)	5.65	4.87	5.12

**Recovery:** The recovery of antigen spiked to levels throughout the range of the assay in blocking buffer was evaluated.

Sample	1	2	3	4
n	4	4	4	4
Mean (ng/ml)	0.871	2.92	8.58	38.3
Average % Recovery	109	117	114	109
Range	103-111%	114-120%	114-116%	106-111%

**Specificity:** This assay recognizes natural mouse C3. Significant cross reaction is observed with pooled normal plasma from rat and rabbit. Pooled normal plasma from human, pig, rabbit, sheep, canine, and horse were assayed for cross-reactivity. No significant cross-reactivity was observed.



## Mouse Total Complement C3 ELISA Kit

**Linearity:** To assess the linearity of the assay, mouse plasma samples containing high concentrations of antigen were serially diluted to produce samples with values within the dynamic range of the assay.

Sample	1:2	1:4	1:8	1:16
n	4	4	4	4
Average % of expected	99	99	101	105
Range	98-101%	97-102%	99-102%	104-106%

**Sample Values:** Samples were evaluated for the presence of the antigen at varying dilutions.

Sample Type	Dilution	Mean (µg/ml)
Citrate Plasma	1:50,000	893
	1:100,000	893
	1:200,000	905
	1:400,000	943

**Example of ELISA Plate Layout: 20 Standard wells, 76 Sample wells**

	1	2	3	4	5	6	7	8	9	10	11	12
A	0	0.2 ng/ml	0.5 ng/ml	1 ng/ml	2 ng/ml	5 ng/ml	10 ng/ml	20 ng/ml	50 ng/ml	100 ng/ml		
B	0	0.2 ng/ml	0.5 ng/ml	1 ng/ml	2 ng/ml	5 ng/ml	10 ng/ml	20 ng/ml	50 ng/ml	100 ng/ml		
C												
D												
E												
F												
G												
H												

**Disclaimer:** This information is believed to be correct but does not claim to be all-inclusive and should be used only as a guide. The supplier of this kit shall not be held liable for any damage resulting from handling or from contact with the above product.

**NOT FOR HUMAN USE. FOR RESEARCH ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.**



**Cell Sciences®**  
65 Parker Street  
Unit 11  
Newburyport, MA 01950

Toll Free: 888 769-1246  
Phone: 978 572-1070  
Fax: 978 992-0298

E-mail: [info@cellsciences.com](mailto:info@cellsciences.com)  
Web Site: [www.cellsciences.com](http://www.cellsciences.com)